TENSIOMED®

Settings of
Bluetooth Communication Adapter

For Microsoft Windows XP/Vista/7

User's manual

Please read the user's manual carefully before the first use

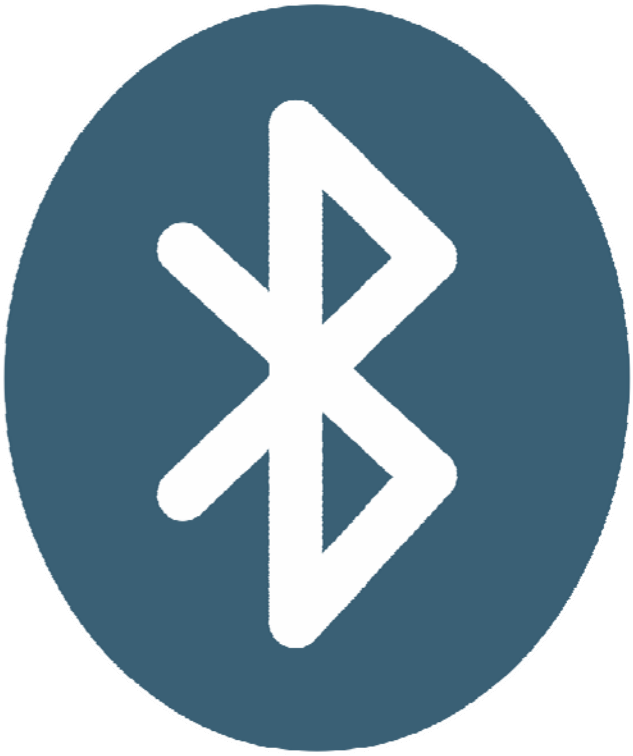

Bluetooth

Table of Contents

1. **Settings of Bluetooth communication adapter for Microsoft XP operation system**.....4

1.1. **Install Bluetooth adapters** 4
1.2. **Install TensioMed Devices** 5

2. **Settings of Bluetooth communication adapter for Microsoft Vista operation system**.....10

2.1. **Install Bluetooth adapters** 10
2.2. **Install TensioMed Devices** 11

1. Settings of Bluetooth communication adapter for Microsoft XP operation system

1.1. Install Bluetooth adapters

Connect the Bluetooth adapter to the PC.

It can be easily done be connecting the adapter to a USB port. (In case your PC is supplied with a built-in Bluetooth adapter or it has already been connected before then the previous instruction should be abandoned).

The Bluetooth adapter will automatically be recognized by Windows XP and the installation of the requisite control programs will be accomplished respectively.

After the connection between Bluetooth and the PC has been established, Bluetooth appears as an addition to system devices (Start > Control panel > System > Device manager; see also Figure1.). Make sure that it contains the option of “Microsoft Bluetooth Enumerators”. (In case the PC has already been provided by Bluetooth communication adapter and additional adapters were unnecessary to connect and install, the previous support is still highly recommended).

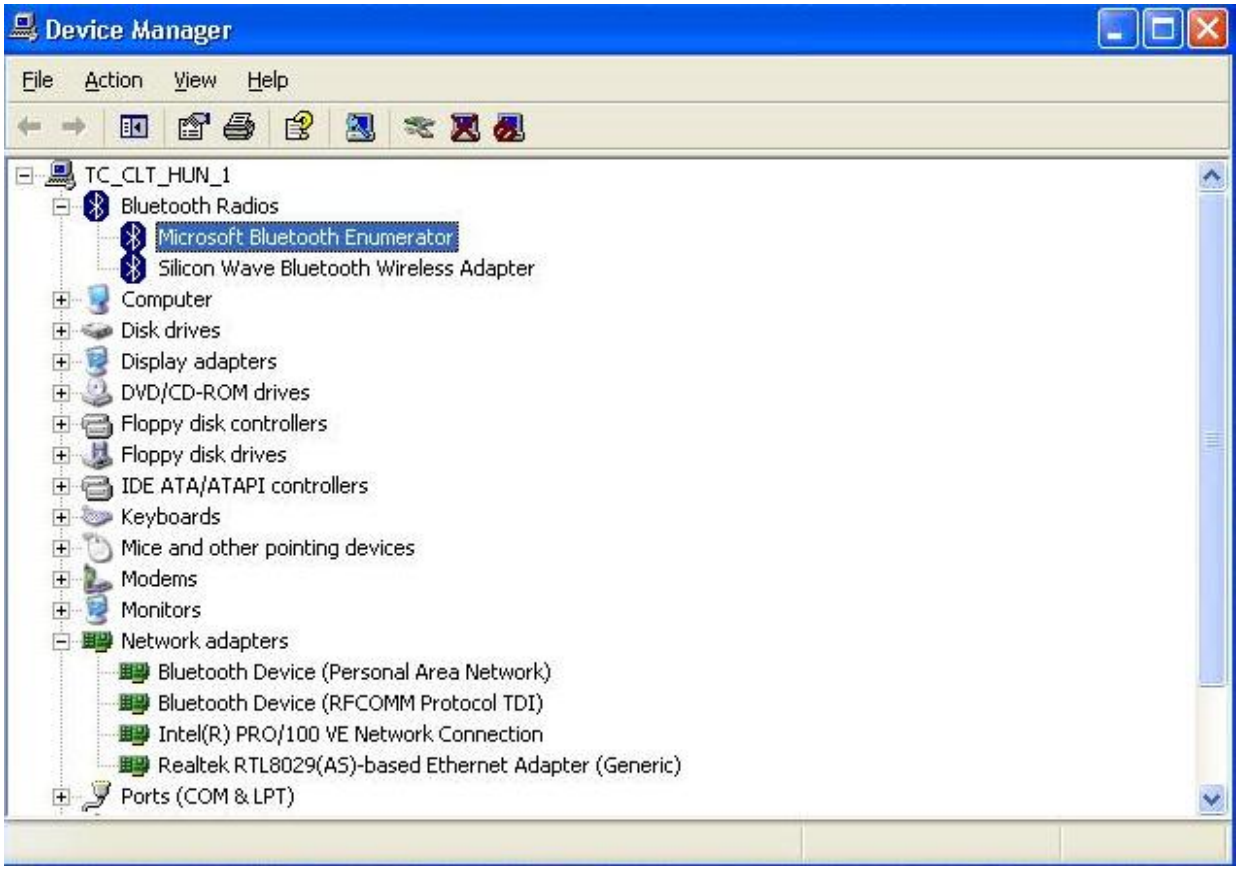

Figure1.

1.2. Install TensioMed Devices

The Bluetooth Utility in the Control Panel enables you to install the required TensioMed device. In case the wireless Bluetooth technology has already been installed to the PC, follow the instructions:

1. Click on the “Start” button, then on “Control Panel” and finally on “Bluetooth Devices”.
2. Select “Add” (Figure2.)

NOTE: If you have further in-use Bluetooth devices e.g.: cell phone or other PC, the following list will contain all the options (Figure2).

Figure2.

Set up the required TensioMed device, select it in the checkbox and press “Next” in the following window (Figure3.)

Add Bluetooth Device Wizard
Welcome to the Add Bluetooth Device Wizard
Before proceeding, refer to the "Bluetooth" section of the device documentation. Then set up your device so that your computer can find it:
- Turn it on
- Make it discoverable (visible)
- Give it a name (optional)
- Press the button on the bottom of the device (keyboards and mice only)
My device is set up and ready to be found.
Add only Bluetooth devices that you trust.
< Back
Next >
Cancel

Figure3.

If the connection between the blood pressure device and the PC has been established, select the device from the list and press “Next” (Figure4.)

Add Bluetooth Device Wizard
Select the Bluetooth device that you want to add.
TensioDay TD3 06/TD0001
New device
New device
If you don't see the device that you want to add, make sure that it is turned on. Follow the setup instructions that came with the device, and then click Search Again.
Search Again
< Back
Next >
Cancel

Figure4.

After choosing “Use the passkey found in the documentation” the passkey must be entered, in the case of blood pressure monitor: 0000 (Figure5.)

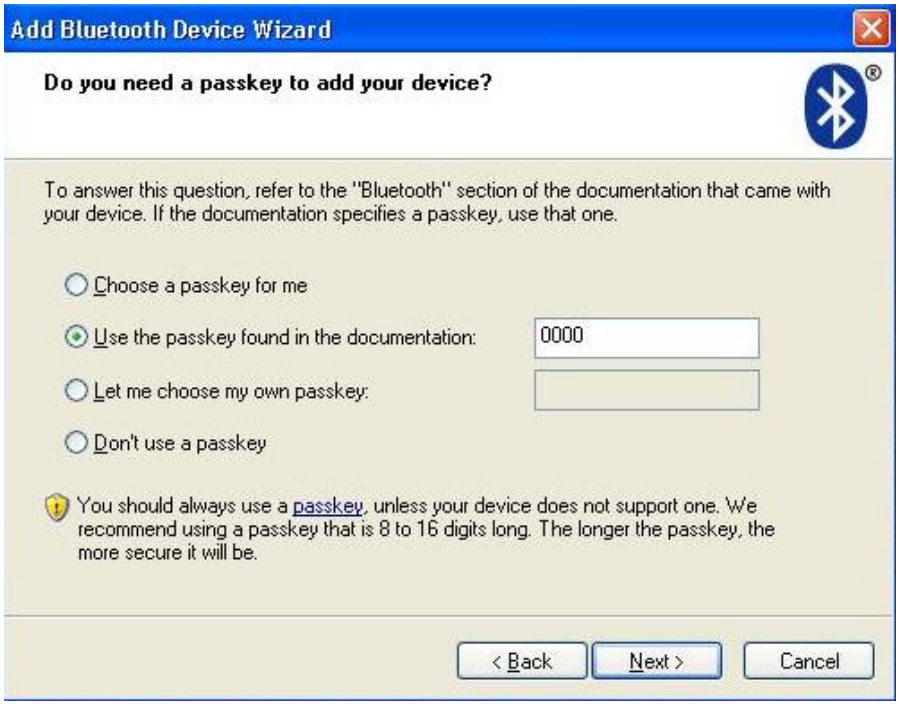
Add Bluetooth Device Wizard
Do you need a passkey to add your device?
To answer this question, refer to the "Bluetooth" section of the documentation that came with your device. If the documentation specifies a passkey, use that one.
Choose a passkey for me
Use the passkey found in the documentation:
0000
Let me choose my own passkey:
Don't use a passkey
You should always use a passkey, unless your device does not support one. We recommend using a passkey that is 8 to 16 digits long. The longer the passkey, the more secure it will be.
< Back
Next >
Cancel

Figure5.

If it is done, press “Next” again, so the setting up process will automatically continue (Figure6.)

Add Bluetooth Device Wizard
Windows is exchanging passkeys.
When instructed below, enter the passkey using your Bluetooth device.
For more information about entering a passkey, see the documentation that came with your device.
Connecting...
Please enter the passkey on your Bluetooth device now.
Passkey: 0000
Installing Bluetooth device...
< Back
Next >
Cancel

Figure6.

To complete installation select “Finish” (Figure7.)

Add Bluetooth Device Wizard
Completing the Add Bluetooth Device Wizard
The Bluetooth device was successfully connected to your computer. Your computer and the device can communicate whenever they are near each other.
These are the COM (serial) ports assigned to your device.
Outgoing COM port: COM6
Learn more about Bluetooth COM ports.
To close this wizard, click Finish.
< Back
Finish
Cancel

Figure7.

If the installation process completed successfully, the exact name of the blood pressure monitoring device will be displayed in the list of Bluetooth Devices (Figure8.)

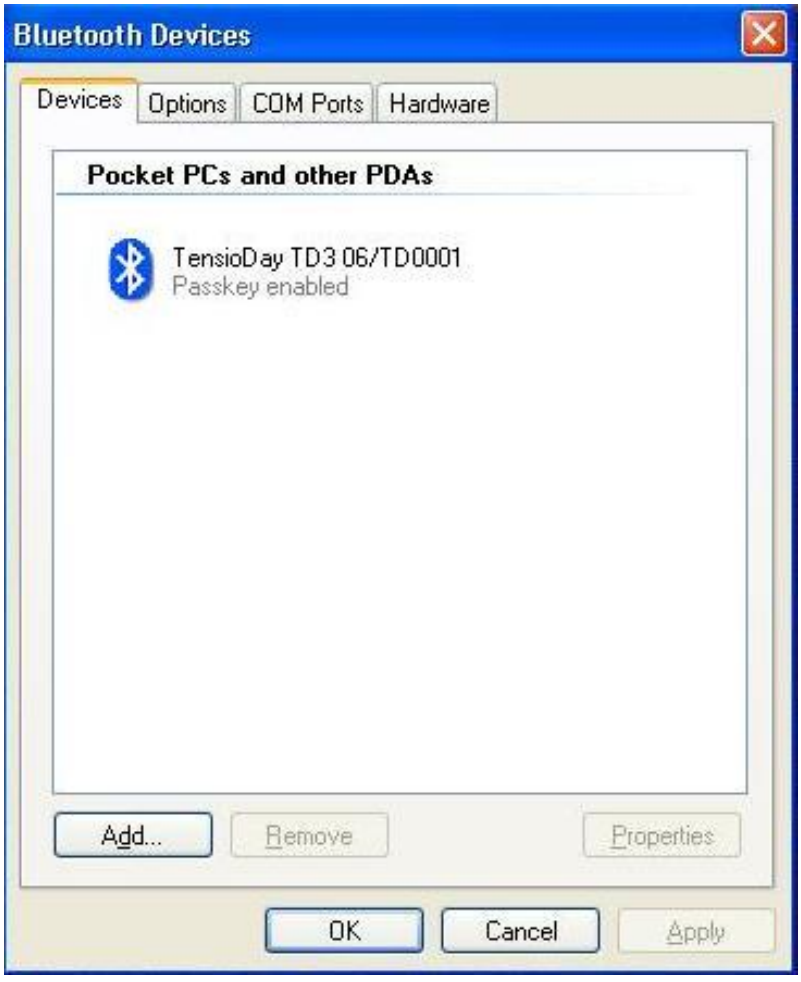

Figure8.

If you have more than one TensioMed devices, now you can add those one by one.
The devices can be distinguished easily by their names in the list showing the product numbers as well (the product number can be found at the bottom of the device e.g.: 06/TD0001).

By clicking on “COM Ports” the user can get to know which virtual communication port was assigned to the required device by the operation system (Figure 9.)

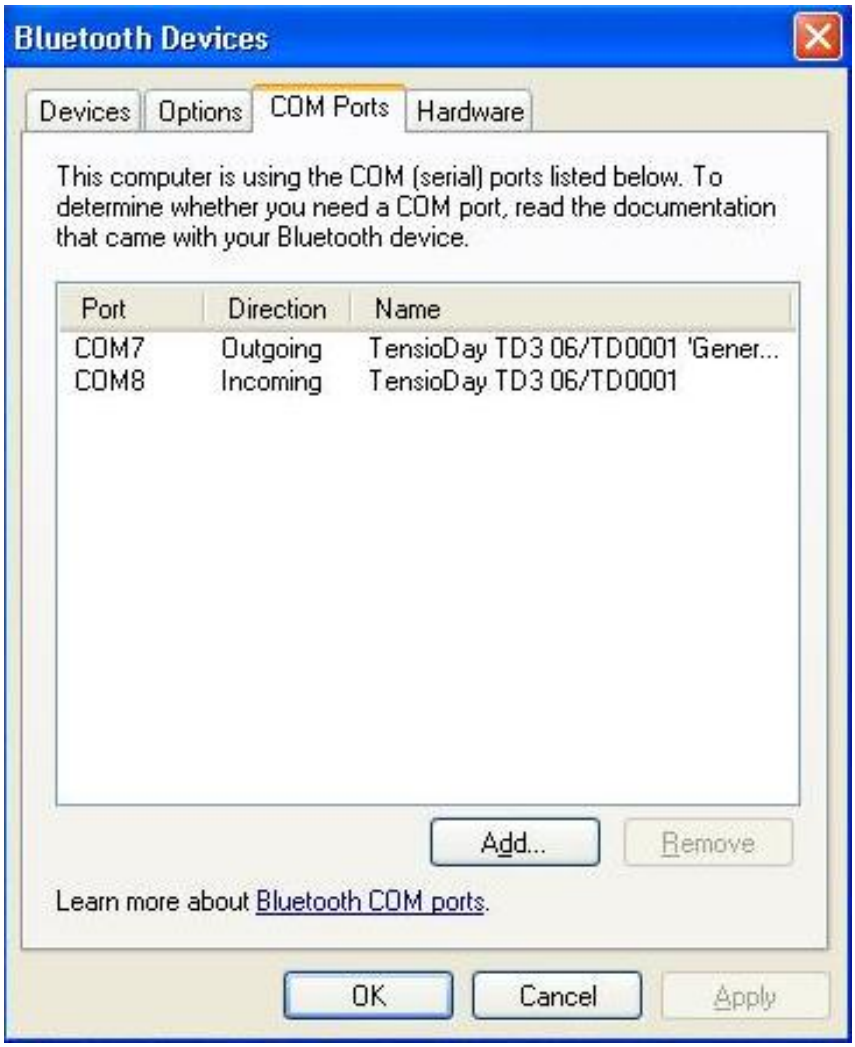

Figure9.

The installation and set up of the Bluetooth Communication port have been completed. Now the PC is ready to send and receive data to and from the TensioMed device.

2. Settings of Bluetooth communication adapter for Microsoft Vista operation system

2.1. Install Bluetooth adapters

Connect the Bluetooth adapter to the PC.

It can be easily done be connecting the adapter to a USB port. (In case your PC is supplied with a built-in Bluetooth adapter or it has already been connected before then the previous instruction should be abandoned).

The Bluetooth adapter will automatically be recognized by Windows Vista and the installation of the requisite control programs will be accomplished respectively.

After the connection between Bluetooth and the PC has been established, Bluetooth appears as an addition to system devices (Start > Control panel > System > Device manager; see also Figure1.). Make sure that it contains the option of “Microsoft Bluetooth Enumerator”. (In case the PC has already been provided by Bluetooth communication adapter and additional adapters were unnecessary to connect and install, the previous support is still highly recommended).

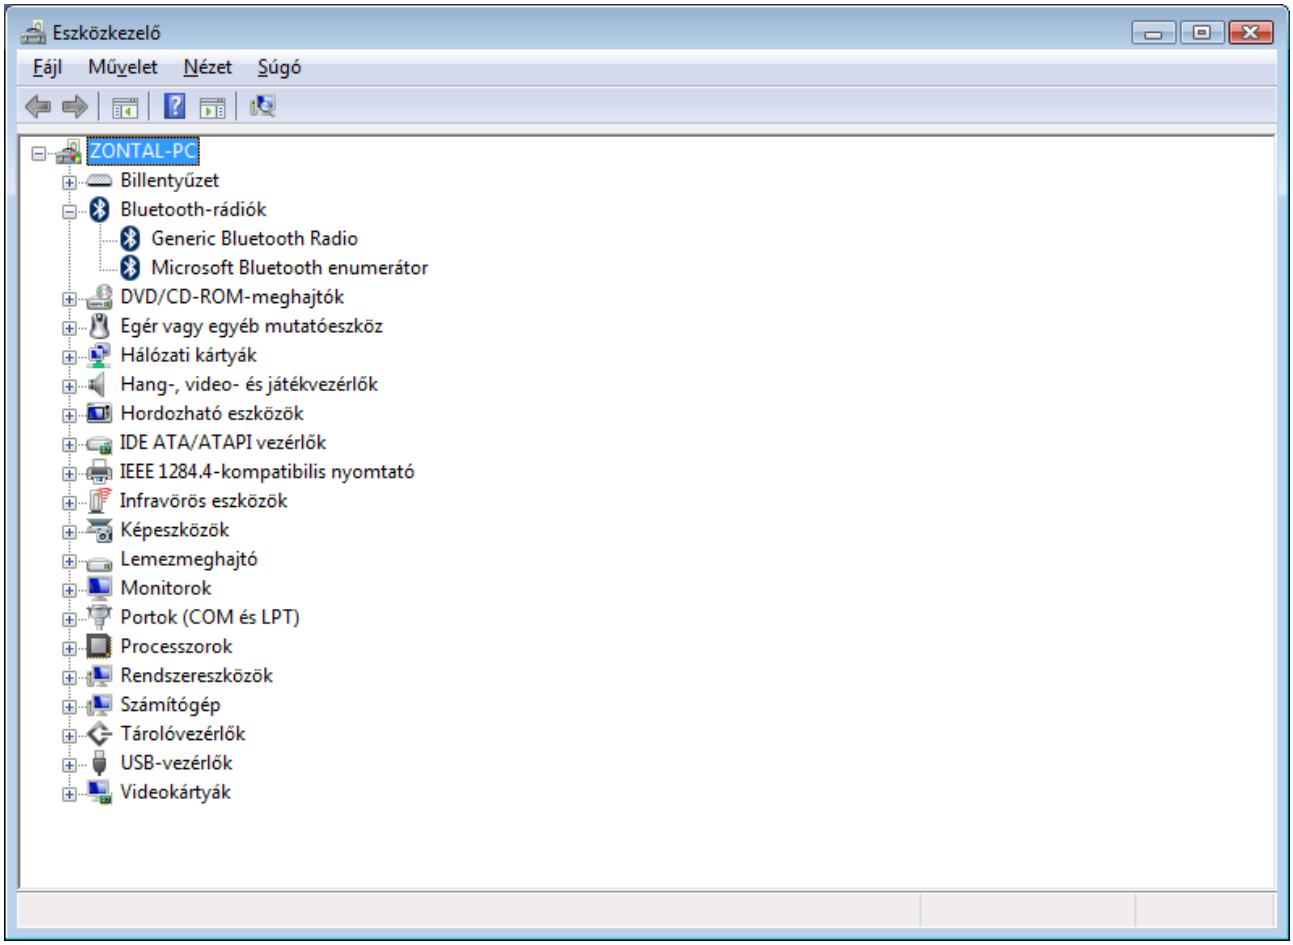

Figure1.

2.2. Install TensioMed Devices

The Bluetooth Utility in the Control Panel enables you to install the required TensioMed device. In case the wireless Bluetooth technology has already been installed to the PC, follow the instructions:

1. Click on the “Start” button, then on “Control Panel” and on the “Hardware and sound” icon. Finally select “Bluetooth devices”.
2. Select “Add wireless device” (Figure2.)

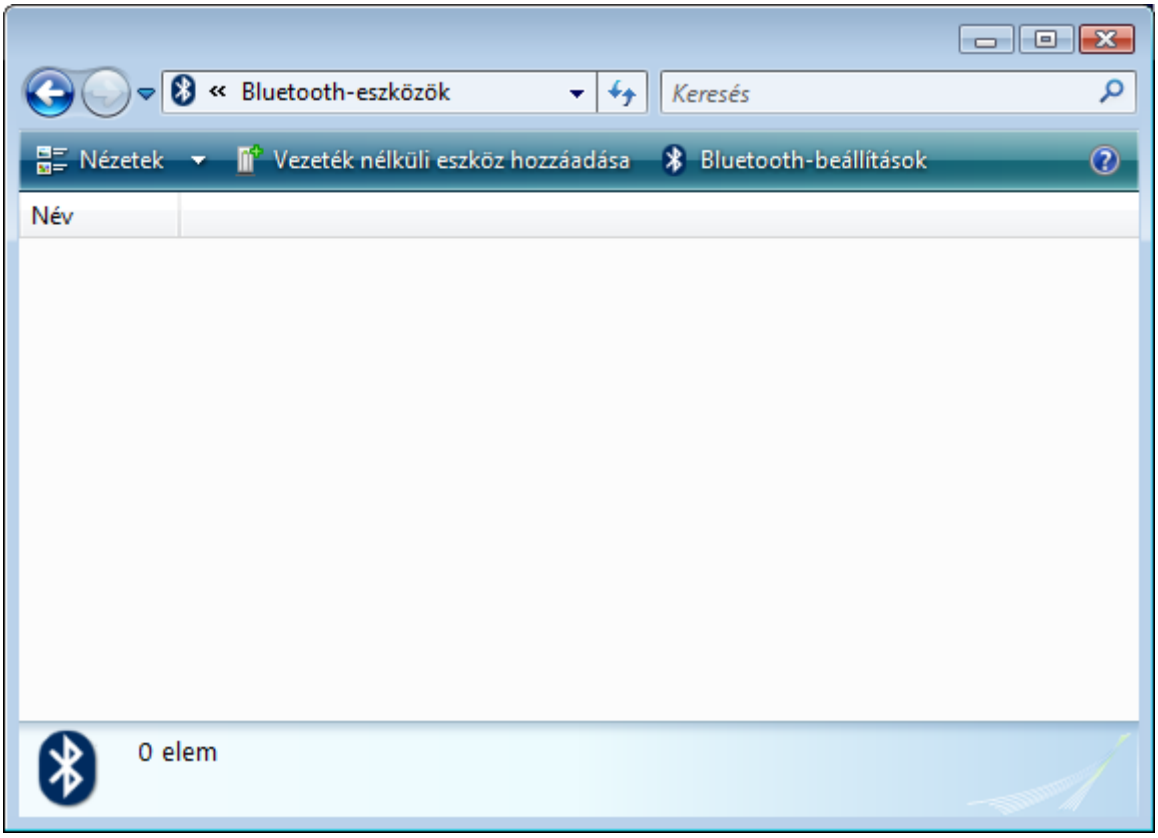

Figgure2.

Set up the required TensioMed device. After the PC successfully established the connection to the device, select it in the checkbox and press “Next” in the following window (Figure3.)
NOTE: If you have further in use Bluetooth devices e.g.: cell phone or other PC, the following list will contain all the options.

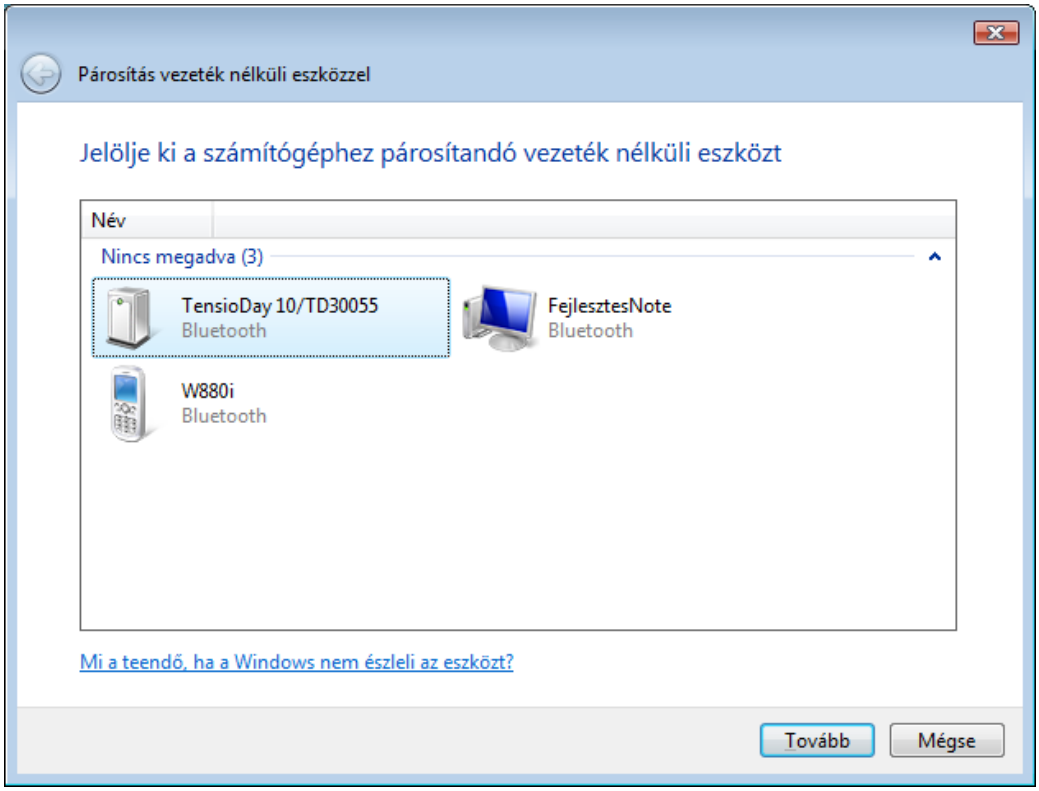

Figure3.

If the connection between the blood pressure device and the PC has been established, select the device in the list and press “Next” (Figure4.)

After choosing “Enter passkey found in the documentation” the passkey must be entered, in the case of blood pressure monitor: 0000 (Figure5.)

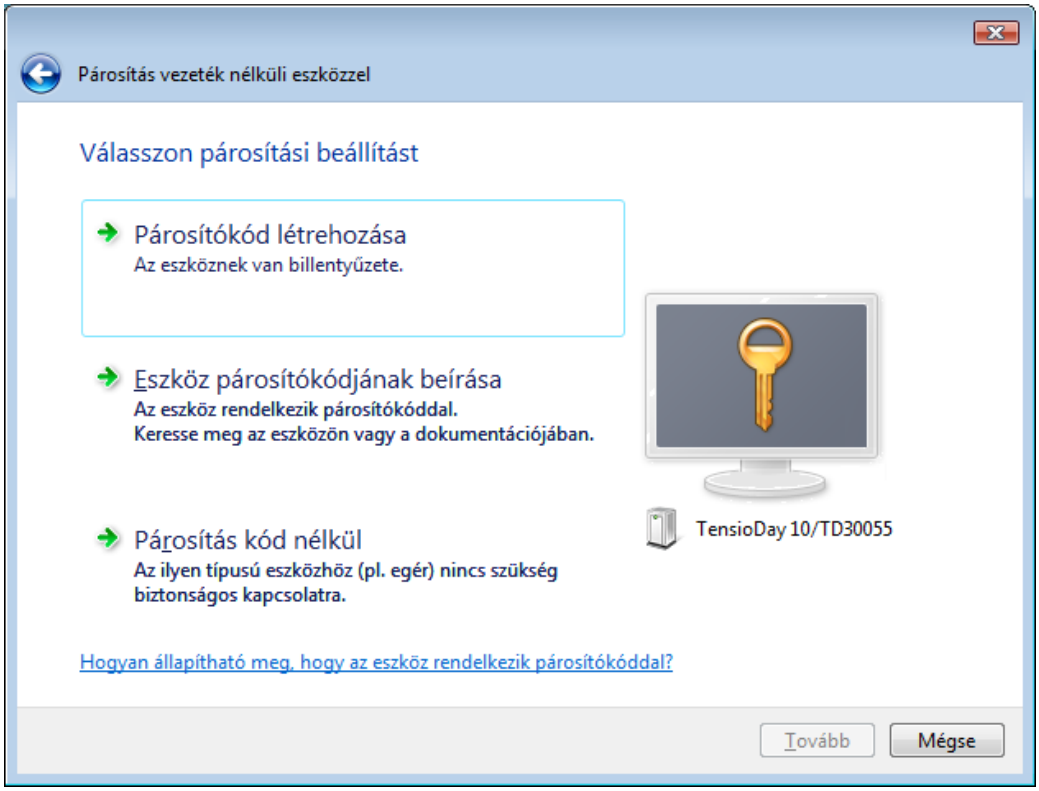
Párosítás vezeték nélküli eszközzel
Válasszon párosítási beállítást
Párosítókód létrehozása
Az eszköznek van billentyűzete.
Eszköz párosítókódjának beírása
Az eszköz rendelkezik párosítókóddal.
Keresse meg az eszközön vagy a dokumentációjában.
Párosítás kód nélkül
Az ilyen típusú eszközhöz (pl. egér) nincs szükség biztonságos kapcsolatra.
TensioDay 10/TD30055
Hogyan állapítható meg, hogy az eszköz rendelkezik párosítókóddal?
Tovább
Mégse

Figure4.

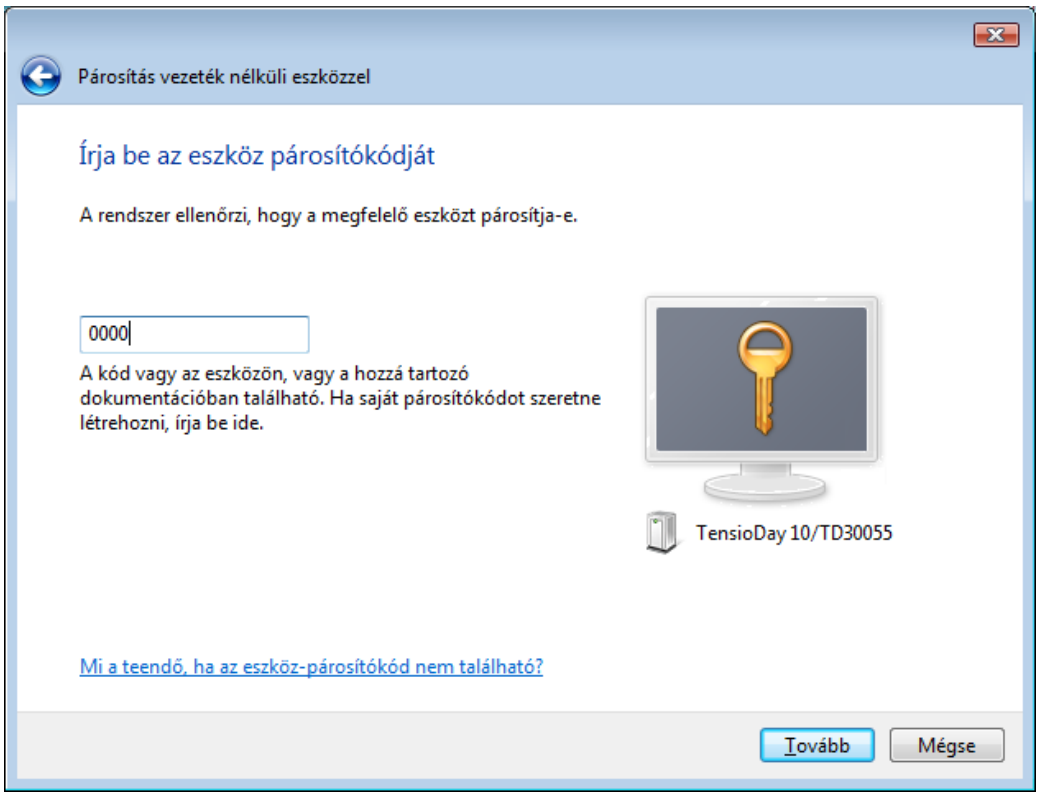
Párosítás vezeték nélküli eszközzel
Írja be az eszköz párosítókódját
A rendszer ellenőrzi, hogy a megfelelő eszközt párosítja-e.
0000
A kód vagy az eszközön, vagy a hozzá tartozó dokumentációban található. Ha saját párosítókódot szeretne létrehozni, írja be ide.
TensioDay 10/TD30055
Mi a teendő, ha az eszköz-párosítókód nem található?
Tovább
Mégse

Figure5.

If it is done, press “Next” again, thus the setting up process will automatically continue.

To complete installation select “Finish” (Figure 6.)

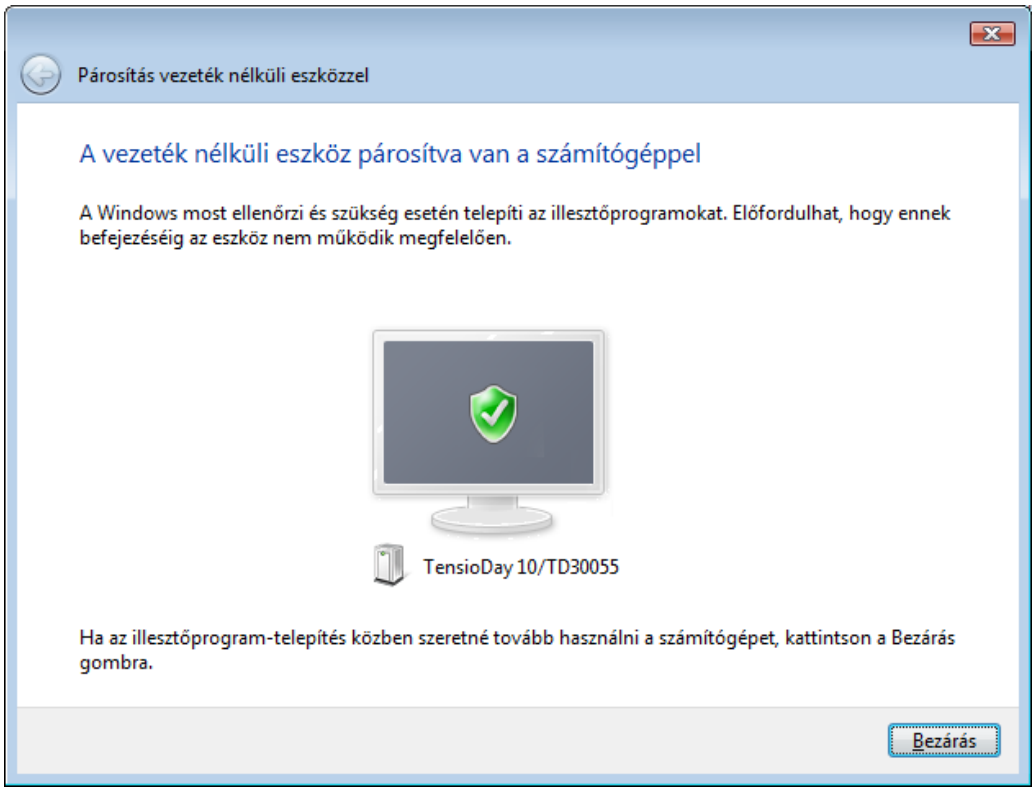
Párosítás vezeték nélküli eszközzel
A vezeték nélküli eszköz párosítva van a számítógéppel
A Windows most ellenőrzi és szükség esetén telepíti az illesztőprogramokat. Előfordulhat, hogy ennek befejezéséig az eszköz nem működik megfelelően.
TensioDay 10/TD30055
Ha az illesztőprogram-telepítés közben szeretné tovább használni a számítógépet, kattintson a Bezárás gombra.
Bezárás

Figure6.

If the installation process completed successfully, the exact name of the blood pressure monitoring device will be displayed in the list of Bluetooth Devices (Figure7.)

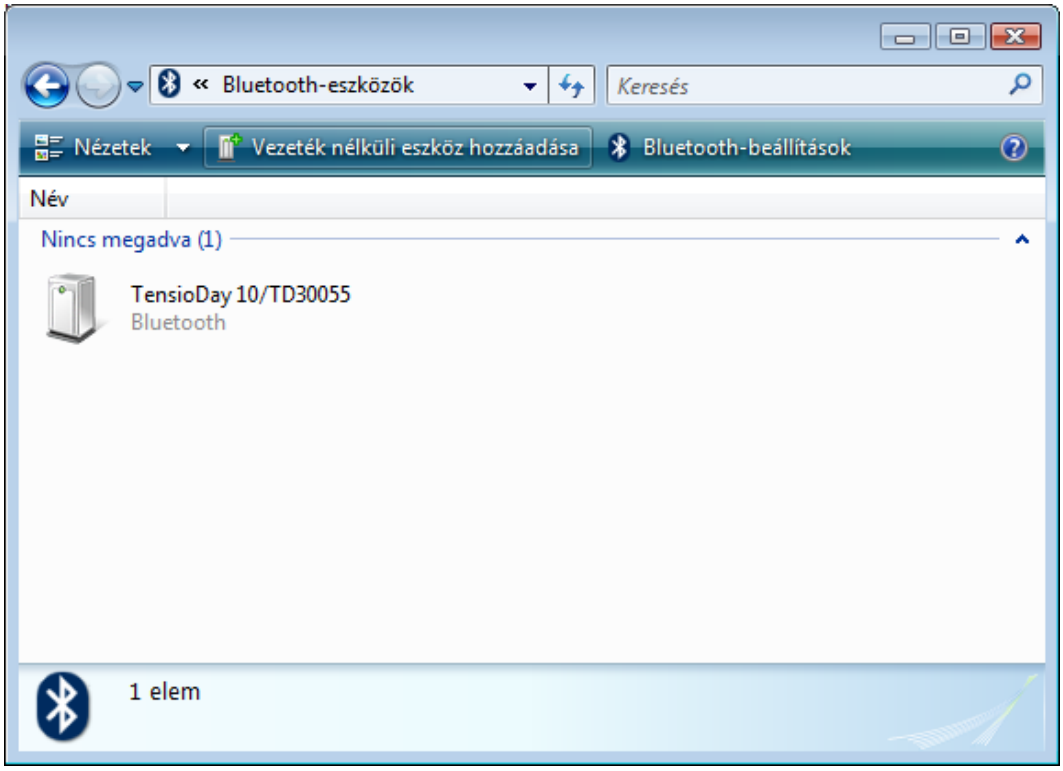

Figure7.

If you have more than one TensioMed devices, now you can add those one by one.

The devices can be distinguished easily by their names in the list showing the product numbers as well (the product number can be found at the bottom of the device e.g.: 06/TD0001).

By clicking on “COM Ports” the user can get to know which virtual communication port was assigned to the required device by the operation system (Figure 8.)

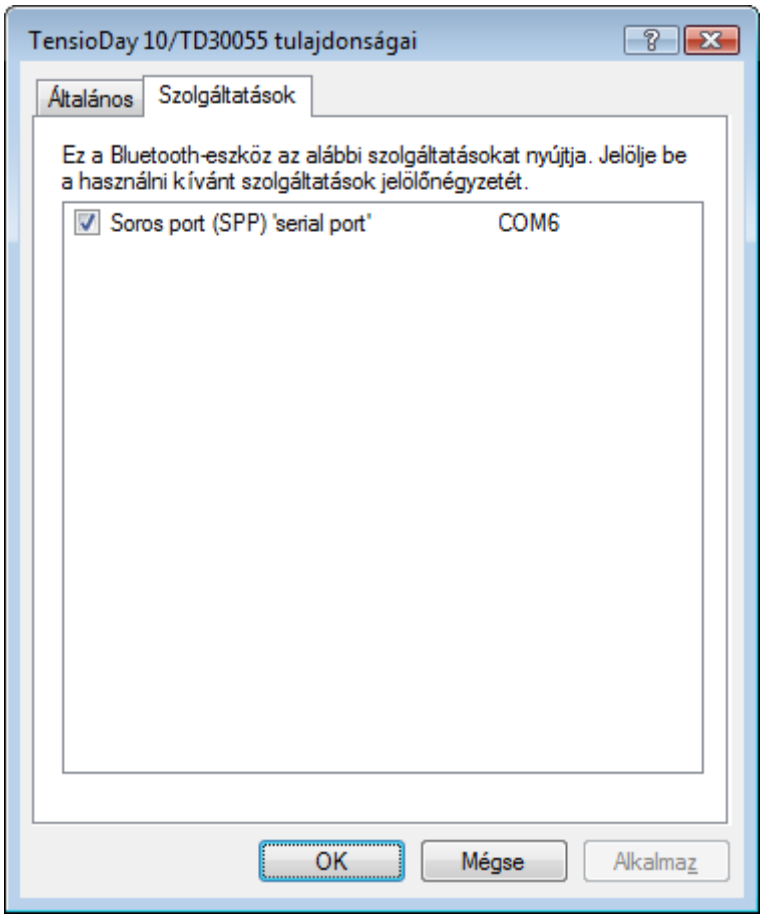

Figure8.

The installation and set up of the Bluetooth Communication port have been completed. Now the PC is ready to send and receive data to and from the TensioMed device.

TENSIOMED®